



Certificado No.:


67153

Registrador de Temperatura y Humedad

Fecha de Calibración:

2026-03-14

Queclink

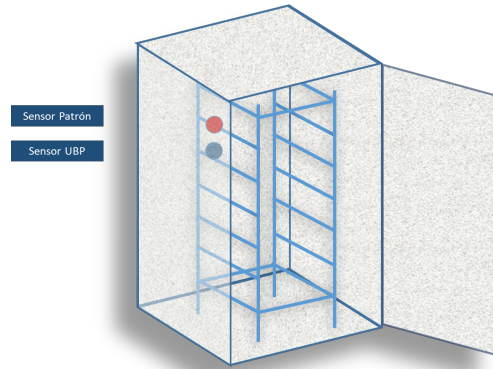

UBICACION DE EQUIPOS PATRON

Tabla 1.0: Lecturas de la TEMPERATURA en el área de trabajo (°C)

Tiempo (hh:mm:ss)	Temperatura Patrón (°C)	Temperatura Calibrando (°C)	Error (°C)
9:30:00 AM	16.20	15.80	-0.40
9:32:00 AM	16.40	15.40	-1.00
9:34:00 AM	16.80	15.90	-0.90
9:36:00 AM	16.90	15.70	-1.20
9:38:00 AM	16.10	15.47	-0.63
9:40:00 AM	16.00	15.10	-0.90
9:42:00 AM	15.80	15.00	-0.80
9:44:00 AM	15.40	14.80	-0.60
9:46:00 AM	15.20	14.90	-0.30
9:48:00 AM	15.10	14.70	-0.40
9:50:00 AM	15.00	14.10	-0.90
9:52:00 AM	14.80	14.80	0.00
9:54:00 AM	14.90	14.90	0.00
9:56:00 AM	14.70	14.70	0.00
9:58:00 AM	14.50	15.00	0.50
10:00:00 AM	14.60	15.10	0.50
10:02:00 AM	14.20	15.20	1.00
10:04:00 AM	14.50	15.30	0.80
10:06:00 AM	14.80	15.40	0.60
10:08:00 AM	14.90	15.10	0.20
10:10:00 AM	15.10	15.30	0.20
10:12:00 AM	15.20	15.80	0.60
10:14:00 AM	15.30	16.00	0.70
10:16:00 AM	15.40	16.10	0.70
10:18:00 AM	15.80	16.00	0.20
10:20:00 AM	16.00	16.40	0.40
10:22:00 AM	16.40	16.80	0.40
10:24:00 AM	16.80	16.90	0.10
10:26:00 AM	16.90	16.40	-0.50
10:28:00 AM	17.00	16.20	-0.80
<b>Promedio</b>	<b>15.56</b>	<b>15.48</b>	
<b>Desviación</b>	<b>0.84</b>	<b>0.67</b>	
<b>Max</b>	<b>17.00</b>	<b>16.90</b>	
<b>Min</b>	<b>14.20</b>	<b>14.10</b>	

Certificado No.:

67153

Registrador de Temperatura y Humedad

Fecha de Calibración:

2026-03-14

Queclink

Tabla 2.0: Lecturas de la HUMEDAD RELATIVA en el área de trabajo (%HR)

Tiempo (hh:mm:ss)	Humedad Relativa Patrón (%HR)	Humedad Relativa Calibrando (%HR)	Error (%HR)
9:30:00 AM	66.10	63.80	-2.30
9:32:00 AM	66.20	63.90	-2.30
9:34:00 AM	66.40	64.00	-2.40
9:36:00 AM	66.80	64.20	-2.60
9:38:00 AM	66.90	64.10	-2.80
9:40:00 AM	66.20	64.50	-1.70
9:42:00 AM	66.00	64.50	-1.50
9:44:00 AM	65.80	64.80	-1.00
9:46:00 AM	65.90	64.90	-1.00
9:48:00 AM	65.70	65.00	-0.70
9:50:00 AM	65.40	65.10	-0.30
9:52:00 AM	65.10	65.20	0.10
9:54:00 AM	65.00	65.30	0.30
9:56:00 AM	64.80	65.70	0.90
9:58:00 AM	64.90	65.80	0.90
10:00:00 AM	64.20	65.90	1.70
10:02:00 AM	64.35	66.10	1.75
10:04:00 AM	64.30	66.20	1.90
10:06:00 AM	64.20	66.30	2.10
10:08:00 AM	64.00	66.40	2.40
10:10:00 AM	64.30	66.80	2.50
10:12:00 AM	63.50	67.10	3.60
10:14:00 AM	63.80	67.00	3.20
10:16:00 AM	63.90	67.10	3.20
10:18:00 AM	64.00	67.20	3.20
10:20:00 AM	64.70	66.50	1.80
10:22:00 AM	64.80	66.20	1.40
10:24:00 AM	64.90	66.30	1.40
10:26:00 AM	64.20	66.10	1.90
10:28:00 AM	64.00	66.80	2.80
<b>Promedio</b>	<b>65.01</b>	<b>65.63</b>	
<b>Desviación</b>	<b>0.97</b>	<b>1.07</b>	
<b>Max</b>	<b>66.90</b>	<b>67.20</b>	
<b>Min</b>	<b>63.50</b>	<b>63.80</b>	

Certificado No.:

67153

Registrador de Temperatura y Humedad

Fecha de Calibración:

2026-03-14

Quealink

