



Certificado No.:


66056

Registrador de Temperatura y Humedad

Fecha de Calibración:

2026-02-10

Maxim

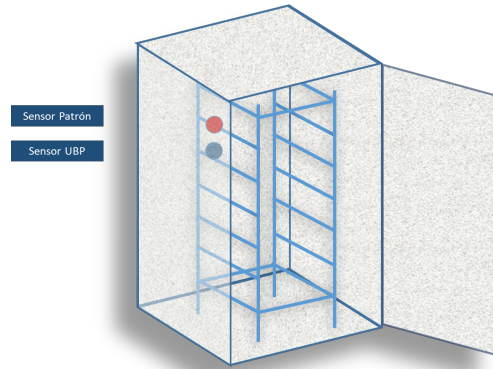

UBICACION DE EQUIPOS PATRON

Tabla 1.0: Lecturas de la TEMPERATURA en el área de trabajo (°C)

Tiempo (hh:mm:ss)	Temperatura Patrón (°C)	Temperatura Calibrando (°C)	Error (°C)
10:20:00 AM	20.2	19.5	-0.7
10:22:00 AM	20.3	19.7	-0.6
10:24:00 AM	20.4	19.7	-0.7
10:26:00 AM	20.0	19.8	-0.2
10:28:00 AM	20.0	19.9	-0.1
10:30:00 AM	19.9	19.5	-0.4
10:32:00 AM	19.8	19.4	-0.4
10:34:00 AM	19.5	19.2	-0.3
10:36:00 AM	19.6	19.0	-0.6
10:38:00 AM	19.4	19.0	-0.4
10:40:00 AM	19.0	18.9	-0.1
10:42:00 AM	19.0	18.7	-0.3
10:44:00 AM	18.5	18.9	0.4
10:46:00 AM	18.6	19.0	0.4
10:48:00 AM	18.9	19.5	0.6
10:50:00 AM	18.7	19.6	0.9
10:52:00 AM	18.9	19.8	0.9
10:54:00 AM	19.0	19.5	0.5
10:56:00 AM	19.0	19.5	0.5
10:58:00 AM	19.2	19.6	0.4
11:00:00 AM	19.5	19.8	0.3
11:02:00 AM	19.6	20.0	0.4
11:04:00 AM	19.8	20.1	0.3
11:06:00 AM	20.0	20.5	0.5
11:08:00 AM	20.3	20.7	0.4
11:10:00 AM	20.5	21.0	0.5
11:12:00 AM	20.8	21.0	0.2
11:14:00 AM	21.0	21.2	0.2
11:16:00 AM	21.0	21.5	0.5
11:18:00 AM	21.2	21.8	0.6
<b>Promedio</b>	<b>19.72</b>	<b>19.84</b>	
<b>Desviación</b>	<b>0.756</b>	<b>0.81</b>	
<b>Max</b>	<b>21.20</b>	<b>21.5</b>	
<b>Min</b>	<b>18.50</b>	<b>18.7</b>	

Certificado No.:

66056

Registrador de Temperatura y Humedad

Fecha de Calibración:

2026-02-10

Maxim

Tabla 2.0: Lecturas de la HUMEDAD RELATIVA en el área de trabajo (%HR)

Tiempo (hh:mm:ss)	Humedad Relativa Patrón (%HR)	Humedad Relativa Calibrando (%HR)	Error (%HR)
10:20:00 AM	61.20	59.41	-1.79
10:22:00 AM	61.50	60.80	-0.70
10:24:00 AM	61.80	60.90	-0.90
10:26:00 AM	61.40	61.20	-0.20
10:28:00 AM	61.00	61.30	0.30
10:30:00 AM	61.00	61.50	0.50
10:32:00 AM	60.50	61.80	1.30
10:34:00 AM	60.30	61.20	0.90
10:36:00 AM	60.20	61.00	0.80
10:38:00 AM	60.10	60.50	0.40
10:40:00 AM	60.00	60.30	0.30
10:42:00 AM	60.00	60.80	0.80
10:44:00 AM	59.80	60.90	1.10
10:46:00 AM	59.80	60.70	0.90
10:48:00 AM	59.70	59.80	0.10
10:50:00 AM	59.40	59.40	0.00
10:52:00 AM	59.20	59.60	0.40
10:54:00 AM	59.10	59.90	0.80
10:56:00 AM	59.00	60.10	1.10
10:58:00 AM	58.80	60.20	1.40
11:00:00 AM	58.90	60.30	1.40
11:02:00 AM	58.70	60.40	1.70
11:04:00 AM	58.90	60.50	1.60
11:06:00 AM	59.00	60.20	1.20
11:08:00 AM	59.80	60.50	0.70
11:10:00 AM	60.00	60.50	0.50
11:12:00 AM	60.20	60.80	0.60
11:14:00 AM	60.30	60.90	0.60
11:16:00 AM	60.80	61.00	0.20
11:18:00 AM	61.20	61.50	0.30
<b>Promedio</b>	<b>60.05</b>	<b>60.60</b>	
<b>Desviación</b>	<b>0.890</b>	<b>0.610</b>	
<b>Max</b>	<b>61.80</b>	<b>61.80</b>	
<b>Min</b>	<b>58.70</b>	<b>59.40</b>	

Certificado No.:

66056

Registrador de Temperatura y Humedad

Fecha de Calibración:

2026-02-10

Maxim

