

Certificado No.:

63337

Registrador de Temperatura y Humedad

Fecha de Calibración:

2025-11-15

AOSONG

Tabla 1.0: Lecturas de la TEMPERATURA en el área de trabajo (°C)

Tiempo (hh:mm:ss)	Temperatura Patrón (°C)	Temperatura Calibrando (°C)	Error (°C)
11:30:00 AM	15.8	15.7	-0.10
11:31:00 AM	15.7	15.0	-0.70
11:32:00 AM	15.6	15.0	-0.60
11:33:00 AM	15.6	15.0	-0.60
11:34:00 AM	15.6	14.8	-0.80
11:35:00 AM	15.6	14.7	-0.90
11:36:00 AM	15.6	14.6	-1.00
11:37:00 AM	15.3	14.8	-0.50
11:38:00 AM	15.1	14.9	-0.20
11:39:00 AM	15.0	14.4	-0.60
11:40:00 AM	15.0	14.3	-0.70
11:41:00 AM	14.8	14.0	-0.80
11:42:00 AM	14.7	14.0	-0.70
11:43:00 AM	14.6	13.8	-0.80
11:44:00 AM	14.8	13.7	-1.10
11:45:00 AM	14.9	13.6	-1.30
11:46:00 AM	14.4	13.8	-0.60
11:47:00 AM	14.4	13.9	-0.50
11:48:00 AM	14.4	14.0	-0.40
11:49:00 AM	14.4	14.3	-0.10
11:50:00 AM	14.4	14.2	-0.20
11:51:00 AM	14.0	14.2	0.20
11:52:00 AM	14.0	14.2	0.20
11:53:00 AM	13.8	14.2	0.40
11:54:00 AM	13.9	14.2	0.30
11:55:00 AM	13.7	14.8	1.10
11:56:00 AM	13.6	14.9	1.30
11:57:00 AM	13.8	15.0	1.20
11:58:00 AM	14.0	15.4	1.40
11:59:00 AM	14.5	15.3	0.80
Promedio	14.70	14.49	
Desviación	0.681	0.545	
Max	15.80	15.70	
Min	13.60	13.60	

Certificado No.:

63337

Registrador de Temperatura y Humedad

Fecha de Calibración:

2025-11-15

AOSONG

Tabla 2.0: Lecturas de la HUMEDAD RELATIVA en el área de trabajo (%HR)

Tiempo (hh:mm:ss)	Humedad Relativa Patrón (%HR)	Humedad Relativa Calibrando (%HR)	Error (%HR)
11:30:00 AM	60.5	57.8	-2.70
11:31:00 AM	60.4	57.9	-2.50
11:32:00 AM	60.4	57.9	-2.50
11:33:00 AM	60.3	57.9	-2.40
11:34:00 AM	60.3	58.3	-2.00
11:35:00 AM	60.3	58.4	-1.90
11:36:00 AM	60.3	58.6	-1.70
11:37:00 AM	60.3	58.6	-1.70
11:38:00 AM	60.3	58.6	-1.70
11:39:00 AM	60.3	58.6	-1.70
11:40:00 AM	60.0	57.9	-2.10
11:41:00 AM	60.0	58.9	-1.10
11:42:00 AM	59.8	59.0	-0.80
11:43:00 AM	59.4	59.0	-0.40
11:44:00 AM	59.3	58.7	-0.60
11:45:00 AM	59.2	58.6	-0.60
11:46:00 AM	59.2	58.4	-0.80
11:47:00 AM	59.2	58.4	-0.80
11:48:00 AM	59.2	58.4	-0.80
11:49:00 AM	59.2	58.3	-0.90
11:50:00 AM	59.2	58.0	-1.20
11:51:00 AM	59.0	58.0	-1.00
11:52:00 AM	59.0	57.9	-1.10
11:53:00 AM	58.7	57.8	-0.90
11:54:00 AM	58.4	57.5	-0.90
11:55:00 AM	58.0	57.8	-0.20
11:56:00 AM	58.0	57.7	-0.30
11:57:00 AM	57.9	57.6	-0.30
11:58:00 AM	57.4	57.4	0.00
11:59:00 AM	57.2	57.9	0.70
Promedio	59.36	58.19	
Desviación	0.961	0.449	
Max	60.50	59.00	
Min	57.20	57.40	

Certificado No.:

63337


Registrador de Temperatura y Humedad

Fecha de Calibración:

2025-11-15

AOSONG

Curva de Calibración - TEMPERATURA

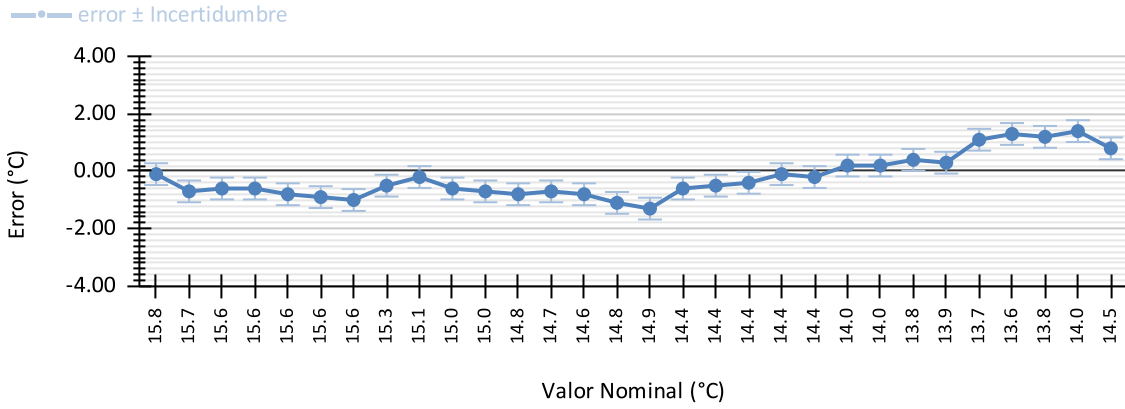

Curva de Calibración - % HUMEDAD RELATIVA

