



Certificado No.:

65550

Registrador de Temperatura y Humedad

Fecha de Calibración:

2026-01-07

HWA-SUNG-THERMO

Tabla 1.0: Lecturas de la TEMPERATURA en el área de trabajo (°C)

Tiempo (hh:mm:ss)	Temperatura Patrón (°C)	Temperatura Calibrando (°C)	Error (°C)
2:30:00 PM	21.0	21.5	0.50
2:31:00 PM	21.5	21.4	-0.10
2:32:00 PM	21.4	21.3	-0.10
2:33:00 PM	21.6	21.8	0.20
2:34:00 PM	21.8	21.9	0.10
2:35:00 PM	21.8	21.5	-0.30
2:36:00 PM	21.5	20.9	-0.60
2:37:00 PM	21.4	20.8	-0.60
2:38:00 PM	21.0	20.7	-0.30
2:39:00 PM	21.0	20.6	-0.40
2:40:00 PM	20.9	20.5	-0.40
2:41:00 PM	20.8	20.4	-0.40
2:42:00 PM	20.5	20.1	-0.40
2:43:00 PM	20.4	20.0	-0.40
2:44:00 PM	20.1	19.8	-0.30
2:45:00 PM	20.0	19.8	-0.20
2:46:00 PM	20.0	19.7	-0.30
2:47:00 PM	19.8	19.7	-0.10
2:48:00 PM	19.5	19.6	0.10
2:49:00 PM	19.2	19.5	0.30
2:50:00 PM	19.1	19.5	0.40
2:51:00 PM	19.0	19.2	0.20
2:52:00 PM	18.5	19.1	0.60
2:53:00 PM	18.9	19.0	0.10
2:54:00 PM	18.6	19.0	0.40
2:55:00 PM	18.2	18.8	0.60
2:56:00 PM	18.1	18.9	0.80
2:57:00 PM	18.7	19.0	0.30
2:58:00 PM	18.9	19.5	0.60
2:59:00 PM	19.0	19.3	0.30
<b>Promedio</b>	<b>20.07</b>	<b>20.09</b>	
<b>Desviación</b>	<b>1.190</b>	<b>0.951</b>	
<b>Max</b>	<b>21.80</b>	<b>21.90</b>	
<b>Min</b>	<b>18.10</b>	<b>18.80</b>	

Certificado No.:

65550

Registrador de Temperatura y Humedad

Fecha de Calibración:

2026-01-07

HWA-SUNG-THERMO

Tabla 2.0: Lecturas de la HUMEDAD RELATIVA en el área de trabajo (%HR)

Tiempo (hh:mm:ss)	Humedad Relativa Patrón (%HR)	Humedad Relativa Calibrando (%HR)	Error (%HR)
2:30:00 PM	64.5	63.5	-1.00
2:31:00 PM	64.8	63.4	-1.40
2:32:00 PM	64.9	63.5	-1.40
2:33:00 PM	64.5	63.8	-0.70
2:34:00 PM	64.2	63.9	-0.30
2:35:00 PM	64.1	64.0	-0.10
2:36:00 PM	64.0	64.0	0.00
2:37:00 PM	63.8	64.1	0.30
2:38:00 PM	63.9	64.2	0.30
2:39:00 PM	63.7	64.5	0.80
2:40:00 PM	63.4	64.8	1.40
2:41:00 PM	63.8	64.9	1.10
2:42:00 PM	63.4	65.0	1.60
2:43:00 PM	63.0	65.1	2.10
2:44:00 PM	63.0	65.3	2.30
2:45:00 PM	62.9	65.8	2.90
2:46:00 PM	62.8	65.1	2.30
2:47:00 PM	62.4	65.4	3.00
2:48:00 PM	62.1	65.8	3.70
2:49:00 PM	62.4	65.2	2.80
2:50:00 PM	62.1	65.0	2.90
2:51:00 PM	62.0	65.0	3.00
2:52:00 PM	61.8	64.2	2.40
2:53:00 PM	61.4	64.0	2.60
2:54:00 PM	61.8	64.7	2.90
2:55:00 PM	62.0	64.8	2.80
2:56:00 PM	62.3	64.5	2.20
2:57:00 PM	62.8	64.0	1.20
2:58:00 PM	62.9	64.0	1.10
2:59:00 PM	63.1	63.9	0.80
<b>Promedio</b>	<b>63.13</b>	<b>64.51</b>	
<b>Desviación</b>	<b>0.979</b>	<b>0.674</b>	
<b>Max</b>	<b>64.90</b>	<b>65.80</b>	
<b>Min</b>	<b>61.40</b>	<b>63.40</b>	

Certificado No.:

65550


Registrador de Temperatura y Humedad

Fecha de Calibración:

2026-01-07

HWA-SUNG-THERMO

### Curva de Calibración - TEMPERATURA

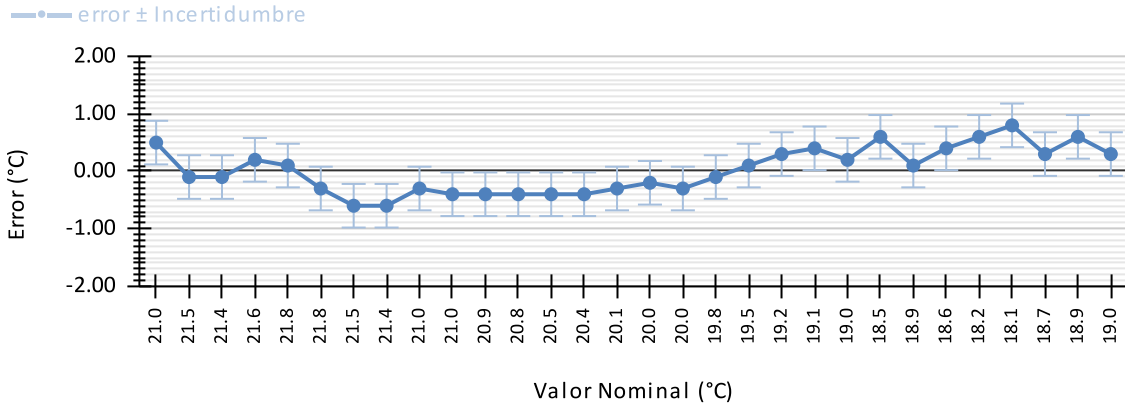

### Curva de Calibración - % HUMEDAD RELATIVA

