



Certificado No.:

65581

Registrador de Temperatura y Humedad

Fecha de Calibración:

2026-01-28

TRACKLINK

Tabla 1.0: Lecturas de la TEMPERATURA en el área de trabajo (°C)

Tiempo (hh:mm:ss)	Temperatura Patrón (°C)	Temperatura Calibrando (°C)	Error (°C)
8:45:00 AM	17.8	18.2	0.40
8:46:00 AM	17.8	18.2	0.40
8:47:00 AM	17.8	18.2	0.40
8:48:00 AM	17.8	18.2	0.40
8:49:00 AM	17.8	18.2	0.40
8:50:00 AM	17.8	18.2	0.40
8:51:00 AM	17.9	18.5	0.60
8:52:00 AM	17.9	18.5	0.60
8:53:00 AM	17.9	18.5	0.60
8:54:00 AM	17.9	18.5	0.60
8:55:00 AM	17.9	18.5	0.60
8:56:00 AM	17.9	18.5	0.60
8:57:00 AM	17.9	18.5	0.60
8:58:00 AM	18.0	18.5	0.50
8:59:00 AM	18.0	18.5	0.50
9:00:00 AM	18.0	18.5	0.50
9:01:00 AM	18.1	18.5	0.40
9:02:00 AM	18.3	18.5	0.20
9:03:00 AM	18.3	18.5	0.20
9:04:00 AM	18.5	18.5	0.00
9:05:00 AM	18.6	18.5	-0.10
9:06:00 AM	18.7	19.0	0.30
9:07:00 AM	18.8	19.0	0.20
9:08:00 AM	18.7	19.0	0.30
9:09:00 AM	18.4	19.0	0.60
9:10:00 AM	18.2	19.0	0.80
9:11:00 AM	18.1	18.7	0.60
9:12:00 AM	18.3	18.7	0.40
9:13:00 AM	18.5	18.7	0.20
9:14:00 AM	18.6	18.7	0.10
<b>Promedio</b>	<b>18.14</b>	<b>18.6</b>	
<b>Desviación</b>	<b>0.324</b>	<b>0.254</b>	
<b>Max</b>	<b>18.80</b>	<b>19.00</b>	
<b>Min</b>	<b>17.80</b>	<b>18.20</b>	

Certificado No.:

65581

Registrador de Temperatura y Humedad

Fecha de Calibración:

2026-01-28

TRACKLINK

Tabla 2.0: Lecturas de la HUMEDAD RELATIVA en el área de trabajo (%HR)

Tiempo (hh:mm:ss)	Humedad Relativa Patrón (%HR)	Humedad Relativa Calibrando (%HR)	Error (%HR)
8:45:00 AM	57.0	63.6	6.60
8:46:00 AM	56.5	63.6	7.10
8:47:00 AM	55.5	63.6	8.10
8:48:00 AM	55.0	63.6	8.60
8:49:00 AM	55.5	63.6	8.10
8:50:00 AM	54.5	63.6	9.10
8:51:00 AM	54.0	60.0	6.00
8:52:00 AM	53.5	60.0	6.50
8:53:00 AM	53.1	60.0	6.90
8:54:00 AM	53.1	60.0	6.90
8:55:00 AM	52.1	60.0	7.90
8:56:00 AM	53.1	58.9	5.80
8:57:00 AM	54.1	58.9	4.80
8:58:00 AM	55.1	58.9	3.80
8:59:00 AM	55.0	58.9	3.90
9:00:00 AM	54.0	58.9	4.90
9:01:00 AM	54.0	56.8	2.80
9:02:00 AM	53.0	56.8	3.80
9:03:00 AM	52.6	56.8	4.20
9:04:00 AM	52.6	56.8	4.20
9:05:00 AM	52.1	56.8	4.70
9:06:00 AM	52.1	53.7	1.60
9:07:00 AM	51.1	53.7	2.60
9:08:00 AM	52.1	53.7	1.60
9:09:00 AM	53.6	53.7	0.10
9:10:00 AM	54.1	53.7	-0.40
9:11:00 AM	54.1	55.3	1.20
9:12:00 AM	53.1	55.3	2.20
9:13:00 AM	53.1	55.3	2.20
9:14:00 AM	52.1	55.3	3.20
<b>Promedio</b>	<b>53.69</b>	<b>58.3</b>	
<b>Desviación</b>	<b>1.393</b>	<b>3.413</b>	
<b>Max</b>	<b>57.00</b>	<b>63.60</b>	
<b>Min</b>	<b>51.10</b>	<b>53.70</b>	

Certificado No.:

65581


Registrador de Temperatura y Humedad

Fecha de Calibración:

2026-01-28

TRACKLINK

### Curva de Calibración - TEMPERATURA

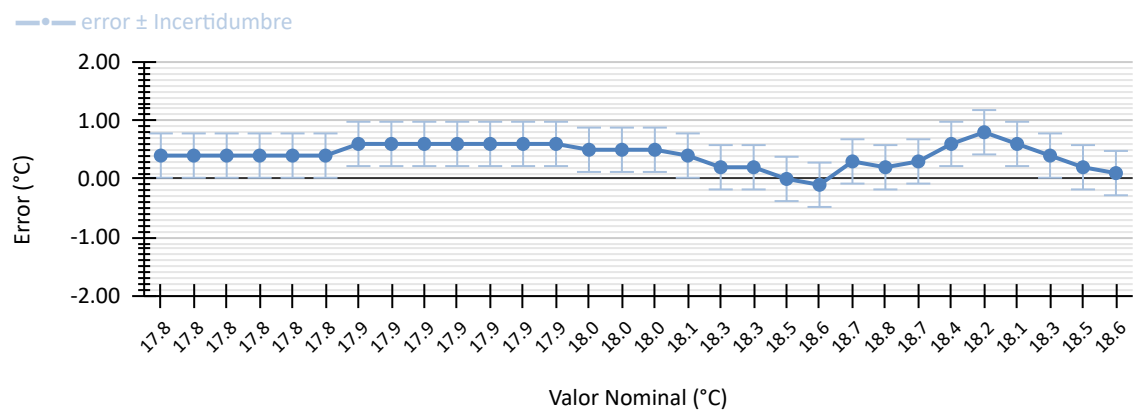

### Curva de Calibración - % HUMEDAD RELATIVA

