

Certificado No.:


66912

Registrador de Temperatura y Humedad

Fecha de Calibración:

2026-03-06

DONGIN THERMO

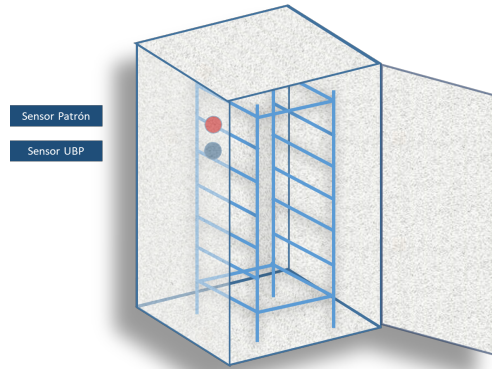

UBICACION DE EQUIPOS PATRON

Tabla 1.0: Lecturas de la TEMPERATURA en el área de trabajo (°C)

Tiempo (hh:mm:ss)	Temperatura Patrón (°C)	Temperatura Calibrando (°C)	Error (°C)
11:00:00 AM	25.8	26.0	0.2
11:01:00 AM	25.9	26.0	0.1
11:02:00 AM	25.7	25.8	0.1
11:03:00 AM	25.6	25.4	-0.2
11:04:00 AM	25.5	25.4	-0.1
11:05:00 AM	25.8	25.1	-0.7
11:06:00 AM	25.9	25.4	-0.5
11:07:00 AM	26.1	25.8	-0.3
11:08:00 AM	26.4	25.4	-1.0
11:09:00 AM	26.5	25.8	-0.7
11:10:00 AM	26.8	26.1	-0.7
11:11:00 AM	25.1	24.7	-0.4
11:12:00 AM	24.8	24.5	-0.3
11:13:00 AM	24.9	24.6	-0.3
11:14:00 AM	24.3	24.2	-0.1
11:15:00 AM	24.2	24.0	-0.2
11:16:00 AM	23.5	24.0	0.5
11:17:00 AM	23.4	23.8	0.4
11:18:00 AM	23.8	23.7	-0.1
11:19:00 AM	23.0	23.4	0.4
11:20:00 AM	22.8	23.5	0.7
11:21:00 AM	22.4	22.8	0.4
11:22:00 AM	22.1	22.9	0.8
11:23:00 AM	22.5	23.0	0.5
11:24:00 AM	23.4	23.1	-0.3
11:25:00 AM	23.5	23.4	-0.1
11:26:00 AM	23.8	23.5	-0.3
11:27:00 AM	24.5	23.8	-0.7
11:28:00 AM	24.9	24.0	-0.9
11:29:00 AM	25.1	24.5	-0.6
Promedio	24.6	24.5	
Desviación	1.340	1.055	
Max	26.80	26.10	
Min	22.10	22.80	

Certificado No.:

66912

Registrador de Temperatura y Humedad

Fecha de Calibración:

2026-03-06

DONGIN THERMO

Tabla 2.0: Lecturas de la HUMEDAD RELATIVA en el área de trabajo (%HR)

Tiempo (hh:mm:ss)	Humedad Relativa Patrón (%HR)	Humedad Relativa Calibrando (%HR)	Error (%HR)
11:00:00 AM	45.7	46.4	0.7
11:01:00 AM	45.6	46.1	0.5
11:02:00 AM	45.5	46.2	0.7
11:03:00 AM	45.4	46.1	0.7
11:04:00 AM	45.1	46.0	0.9
11:05:00 AM	45.0	45.8	0.8
11:06:00 AM	44.8	45.7	0.9
11:07:00 AM	44.9	45.4	0.5
11:08:00 AM	44.7	45.4	0.7
11:09:00 AM	44.5	45.3	0.8
11:10:00 AM	44.1	45.2	1.1
11:11:00 AM	44.2	45.1	0.9
11:12:00 AM	43.8	45.0	1.2
11:13:00 AM	43.7	44.8	1.1
11:14:00 AM	43.5	44.7	1.2
11:15:00 AM	43.2	44.5	1.3
11:16:00 AM	42.5	44.2	1.7
11:17:00 AM	42.8	44.3	1.5
11:18:00 AM	42.1	43.1	1.0
11:19:00 AM	42.5	43.0	0.5
11:20:00 AM	42.8	43.0	0.2
11:21:00 AM	43.1	43.5	0.4
11:22:00 AM	43.5	43.6	0.1
11:23:00 AM	43.8	43.8	0.0
11:24:00 AM	43.9	43.9	0.0
11:25:00 AM	44.1	43.5	-0.6
11:26:00 AM	44.5	43.8	-0.7
11:27:00 AM	44.8	43.9	-0.9
11:28:00 AM	44.9	43.9	-1.0
11:29:00 AM	45.4	44.8	-0.6
Promedio	44.1	44.7	
Desviación	1.021	1.037	
Max	45.70	46.40	
Min	42.10	43.00	

Certificado No.:

66912


Registrador de Temperatura y Humedad

Fecha de Calibración:

2026-03-06

DONGIN THERMO

Curva de Calibración - TEMPERATURA

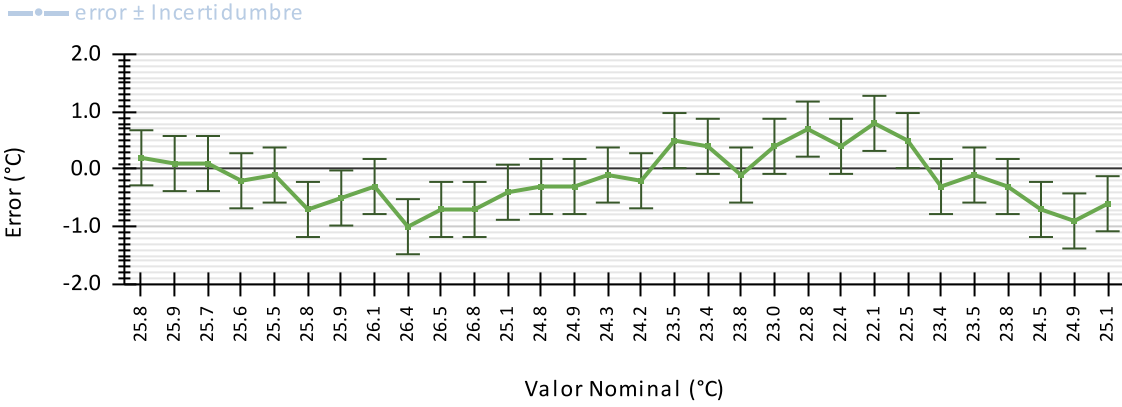

Curva de Calibración - % HUMEDAD RELATIVA

