

Certificado No.:

67229

Registrador de Temperatura y Humedad

Fecha de Calibración:

2026-03-17

Tabla 1.0: Lecturas de la TEMPERATURA en el área de trabajo (°C)

Tiempo (hh:mm:ss)	Temperatura Patrón (°C)	Temperatura Calibrando (°C)	Error (°C)
2:30:00 PM	21.5	21.1	-0.40
2:31:00 PM	21.6	21.0	-0.60
2:32:00 PM	21.8	20.5	-1.30
2:33:00 PM	21.1	20.4	-0.70
2:34:00 PM	21.0	20.6	-0.40
2:35:00 PM	21.0	20.8	-0.20
2:36:00 PM	20.8	20.1	-0.70
2:37:00 PM	20.5	20.0	-0.50
2:38:00 PM	20.6	20.0	-0.60
2:39:00 PM	20.4	20.0	-0.40
2:40:00 PM	20.1	19.8	-0.30
2:41:00 PM	20.0	19.5	-0.50
2:42:00 PM	19.9	19.6	-0.30
2:43:00 PM	19.8	19.7	-0.10
2:44:00 PM	19.5	19.9	0.40
2:45:00 PM	19.4	19.8	0.40
2:46:00 PM	19.8	19.4	-0.40
2:47:00 PM	20.1	19.2	-0.90
2:48:00 PM	20.4	19.5	-0.90
2:49:00 PM	20.5	19.7	-0.80
2:50:00 PM	20.6	19.9	-0.70
2:51:00 PM	20.8	20.1	-0.70
2:52:00 PM	21.1	20.2	-0.90
2:53:00 PM	21.4	20.5	-0.90
2:54:00 PM	21.5	21.1	-0.40
2:55:00 PM	21.6	21.5	-0.10
2:56:00 PM	21.7	21.8	0.10
2:57:00 PM	22.0	22.5	0.50
2:58:00 PM	22.1	22.4	0.30
2:59:00 PM	22.5	22.4	-0.10
Promedio	20.84	20.43	
Desviación	0.816	0.923	
Max	22.50	22.50	
Min	19.40	19.20	

Certificado No.:

67229

Registrador de Temperatura y Humedad

Fecha de Calibración:

2026-03-17

Tabla 2.0: Lecturas de la HUMEDAD RELATIVA en el área de trabajo (%HR)

Tiempo (hh:mm:ss)	Humedad Relativa Patrón (%HR)	Humedad Relativa Calibrando (%HR)	Error (%HR)
2:30:00 PM	60.5	62.8	2.30
2:31:00 PM	60.2	62.5	2.30
2:32:00 PM	60.1	62.4	2.30
2:33:00 PM	60.2	62.1	1.90
2:34:00 PM	60.3	62.0	1.70
2:35:00 PM	60.8	62.1	1.30
2:36:00 PM	60.9	62.4	1.50
2:37:00 PM	61.1	62.9	1.80
2:38:00 PM	61.2	62.4	1.20
2:39:00 PM	61.5	62.1	0.60
2:40:00 PM	61.8	62.9	1.10
2:41:00 PM	62.0	63.1	1.10
2:42:00 PM	62.0	63.2	1.20
2:43:00 PM	62.1	63.4	1.30
2:44:00 PM	62.5	63.5	1.00
2:45:00 PM	62.4	63.8	1.40
2:46:00 PM	62.8	63.2	0.40
2:47:00 PM	62.1	63.1	1.00
2:48:00 PM	61.1	63.0	1.90
2:49:00 PM	61.8	62.8	1.00
2:50:00 PM	61.5	62.5	1.00
2:51:00 PM	61.8	62.4	0.60
2:52:00 PM	61.9	62.1	0.20
2:53:00 PM	61.4	62.5	1.10
2:54:00 PM	61.2	62.8	1.60
2:55:00 PM	61.0	62.9	1.90
2:56:00 PM	60.8	63.0	2.20
2:57:00 PM	60.4	63.1	2.70
2:58:00 PM	60.2	63.2	3.00
2:59:00 PM	60.8	63.4	2.60
Promedio	61.28	62.79	
Desviación	0.765	0.476	
Max	62.80	63.80	
Min	60.10	62.00	

Certificado No.:


67229

Registrador de Temperatura y Humedad

Fecha de Calibración:

2026-03-17

Curva de Calibración - TEMPERATURA

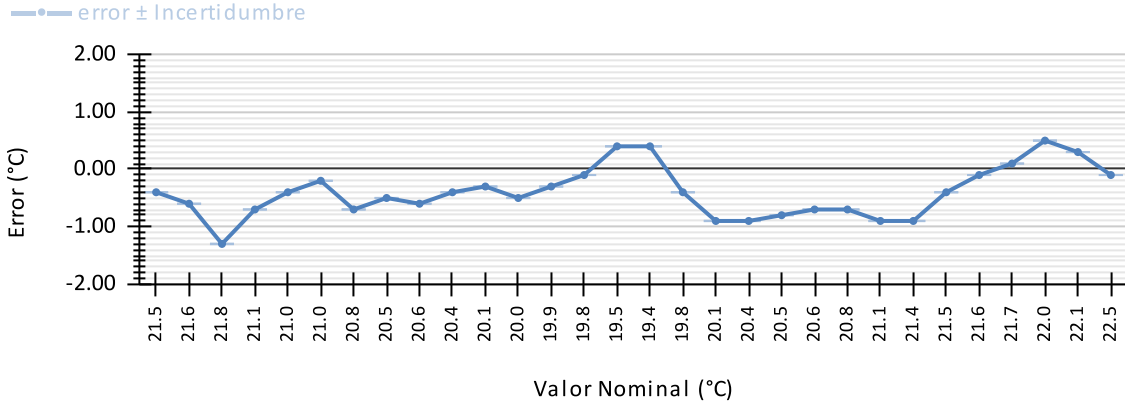

Curva de Calibración - % HUMEDAD RELATIVA

